

Erratum

In the article by Floer M und Meister T, entitled “Endoscopic improvement of the adenoma detection rate during colonoscopy – where do we stand in 2015?” [Digestion 2016;93:202–213, DOI: 10.1159/000442464], the EndoRings seen on Figure 3 was attached from the wrong direction. The corrected figure is shown below:

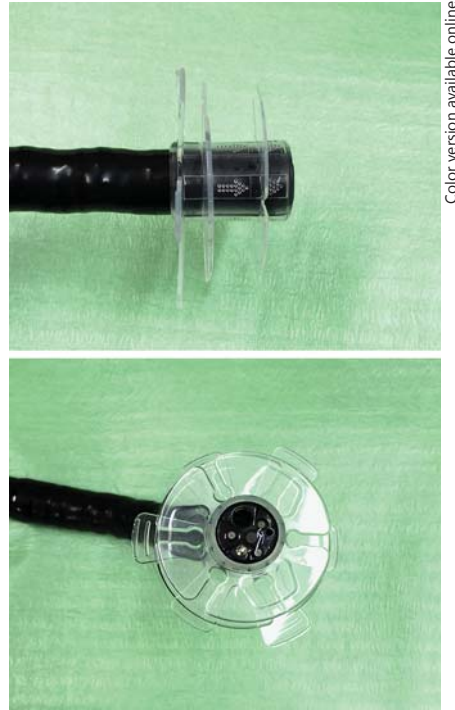


Fig. 3. EndoRings endoscopic add-on device distally attached to the colonoscope (lateral and forward view).